

Operating Handbook

METROTEC

Systems for oxygen measurement

GSM-V6

Oxygen measurement and control unit

Typ GSM

*** Version 2.1 ***

Declaration of Conformity

for
Oxygen measurement and control unit
GSM-V6

This device has been designed for industrial purposes in accordance with:

EN 61000-6-4
EN 61000-6-2

It is compliant with the directives:
EMC Directive: 2014/30/EU
Low Voltage Directive: 2014/35/EU
RoHs: 2011/65/EU

This device complies with following standards:

EN 61010-1
EN 61000-6-4
EN 61000-6-2
EN 63000

Description of measures taken to assure compliance:
Quality management system DIN EN ISO 9001:2015, No. 12 100 27736 TMS

This declaration becomes invalid if changes are made without
our consent.



Kirchheim/Teck, 07.10.2019

Place, Date

Signature

Contents

| | | | | | |
|----------|--|-----------|-----------|----------------------------------|-----------|
| 1 | SAFETY INSTRUCTIONS..... | 4 | 7.1 | Enablement of Configuration .. | 17 |
| 2 | PREFACE | 5 | 7.2 | Displayed values | 18 |
| 3 | INTRODUCTION | 6 | 7.3 | Process parameters | 19 |
| 3.1 | Measurement principle | 6 | 7.4 | mA outputs | 19 |
| 3.2 | Measurement electronics | 7 | 7.5 | Alarm output | 21 |
| 3.3 | Sensor | 7 | 7.6 | Control output..... | 21 |
| 4 | GENERAL ARRANGEMENT | 7 | 7.7 | Scaling of the trend graphs..... | 22 |
| 4.1 | Description of the measurement electronics | 8 | 8 | OPTIONS | 22 |
| 4.2 | Description of the sensor | 8 | 8.1 | Dew point | 22 |
| 4.3 | Sketch of the ducting system .. | 10 | 8.2 | Lambda | 23 |
| 5 | PUTTING THE UNIT INTO OPERATION..... | 11 | 8.3 | CO..... | 23 |
| 5.1 | Switching the unit on | 11 | 8.4 | Calculated oxygen value | 23 |
| 5.2 | Measurement..... | 11 | 9 | INTERFACES | 24 |
| 5.3 | Bottled gases | 11 | 9.1 | Analog interfaces | 24 |
| 5.4 | Process gases | 11 | 9.2 | Digital interfaces | 24 |
| 5.4.1 | General | 11 | 9.2.1 | Standard interfaces | 24 |
| 5.4.2 | Hot process gases..... | 11 | 9.2.2 | Optional interface: RS 485 | 25 |
| 5.4.3 | Special process gases | 11 | 9.2.3 | Optionale interface: | |
| 5.4.4 | Location of condensate collectors | 12 | | Ethernet | 28 |
| 5.4.5 | Filter system arrangement: | 12 | 10 | SPECIAL FEATURES..... | 29 |
| 5.5 | Switching off the measurement unit | 12 | 10.1 | Correction factors | 29 |
| 6 | OPERATION | 13 | 10.2 | Filter factor | 30 |
| 7 | CONFIGURATION..... | 17 | 10.3 | Oxygen controller | 30 |
| | | | 10.4 | Coding | 31 |
| | | | 10.5 | Function of the clock | 31 |
| | | | 11 | TECHNICAL DATA..... | 32 |
| | | | 12 | CONNECTION PLAN..... | 33 |

1 Safety instructions



Please read through this operating manual very carefully before installing and commissioning the unit.

Incorrect utilisation will invalidate the guarantee!



Correct functioning and the operating safety of the unit can only be guaranteed if the ambient conditions specified in the Specifications chapter are maintained.



Only qualified specialists are permitted to commission and operate the unit. The owner of the unit must ensure that the installation complies with the relevant laws and directives. These include, for example, the EU Directives covering safety in the workplace, national safety in the workplace regulations and the prevention of accidents regulations, etc.



You must ensure that the power supplies concur with the details listed on the nameplate. All of the covers needed to ensure that the unit cannot be touched when operating must always be fitted. You must consider the effects of the overall operation and take the necessary precautions if the unit will be linked up with other equipment and/or devices before you switch on.



Parts and surfaces will occasionally become and remain hot during the installation or de-installation. Suitable precautions must be taken in order to prevent injuries or damage to the unit from occurring.



If the unit shows signs of having been damaged and you are of the opinion that that safe operation is no longer possible then you must not run the unit. We recommend that periodical inspections are carried out at our factory or by our customer service department at least once a year.



Future disposal must always comply with the legal regulations.

2 Preface

With the aid of an oxygen sensor , the measurement unit serves to measure the oxygen partial pressure in gaseous atmospheres. Such sensors work at high temperatures and so it is necessary for measures to be taken to ensure that no flammable gas mixtures contact the sensor or the unit. In the event of the sensor ceramic suffering breakage the measurement gas could escape or air could enter the measurement gas side of the unit and so suitable measures have to be taken to avoid such an event leading to environmental pollution or damage being done to equipment.

In the event of incorrect parameters being set or the occurrence of leakage, corrosion, condensation, etc., damage could be done to the equipment and incorrect measurement results be indicated and so it is essential that all parts of equipment be regularly serviced.

The oxygen sensor and its accessories are subjected to thorough quality control in accordance with DIN ISO 9001 in the course of their manufacture and testing.

They must only be installed and used in compliance with all applicable local and special regulations, particularly the VDE and DVGW standards that apply in Germany.

The measurement accuracy and effective function of the measurement device will need to be checked at intervals whose frequency will depend on the application concerned. Such a check must be effected in the course of a calibration and examination check on the equipment being first put into operation.

3 Introduction

3.1 Measurement principle

Oxygen measurement units are designed to process signals transmitted from an oxygen sensor constructed of stabilized zirconium oxide. Zirconium oxide, a ceramic material that is also spoken of as a solid-state electrolyte, acts as an excellent oxygen-ion conductor when at a high temperature.

Within certain temperature limits, that depend on the doping of the material concerned, such ion conductors are able to fill empty spaces in their crystal lattice with oxygen ions. The oxygen ions occur against an electrically conductive surface that is generally of platinum.

The concentration of oxygen in a measurement gas is thus decisive for the extent of oxygen activity, and thus for the number of oxygen ions.

An oxygen sensor consists essentially of a solid-state electrolyte with a contact surface on both sides.

One side of the electrolyte is in contact with a reference gas such as air, and the other with the gas whose oxygen content is to be measured. The mechanical construction of the sensor prevents contact between the two gases so that there is no risk of their being intermixed.

Depending on the application concerned, heated or unheated sensors are used. Unheated sensors are generally used in furnaces while heated sensors are used for applications where the gas to be measured is at a temperature of less than around 600 degrees Celsius (the measurement principle necessitates the sensor being maintained at a temperature of not less than 500 - 650 degrees Celsius).

Heated sensors are maintained at a set temperature by an electronic temperature regulator that forms part of the electronic control unit. The temperature of both heated and unheated sensors as measured by the electronic control is an important parameter for inclusion in the calculation of the oxygen content (oxygen partial pressure) in accordance with the following equation:

$$EMF = \frac{R \cdot T}{4 \cdot F} \cdot \ln\left(\frac{P_1}{P_2}\right)$$

whereby:

- R = 8.31J/mol K
- T = Temperature in Kelvin
- F = 96493 As/mol
- P₁ = Oxygen partial pressure on the reference side with 0.20946 bar
- P₂ = Oxygen partial pressure on the measurement gas side
- EMF = Electromotive force in Volts

3.2 Measurement electronics

The electronic circuit of the measurement unit Type GSM provides the following functions:

Measurement of the oxygen partial pressure

Maintaining the oxygen content at a preset level

Generating alarm signals

Option: Calculation of the dew point

Option: Calculation of the air factor lambda point

The device is operated with the aid of a keypad.

Menus assist the operator in the selection of inputs and outputs and in the setting of parameters.

3.3 Sensor

The sensor of Type A04 is built into the front panel. It includes the actual measurement element of platinum-plated zinc oxide, the heating element needed to heat-up the measurement element to the minimum temperature of 700 degrees Celsius and the thermocouple needed to detect the exact temperature at all times.

The front panel also carries a bypass valve, an illuminated flow meter, gas inlet and outlet connections and also a potentiometer for adjusting the delivery of the gas pump if one is fitted to ensure a flow of the gas whose properties are to be measured.

4 General arrangement



4.1 Description of the measurement electronics

The elements at the front of the unit are in three groups


Keypad:

The keypad has four keys by means of which all the necessary functions can be effected.

Display:

The graphic display provides for the display of measured values, data, time graphs and messages.

4.2 Description of the sensor

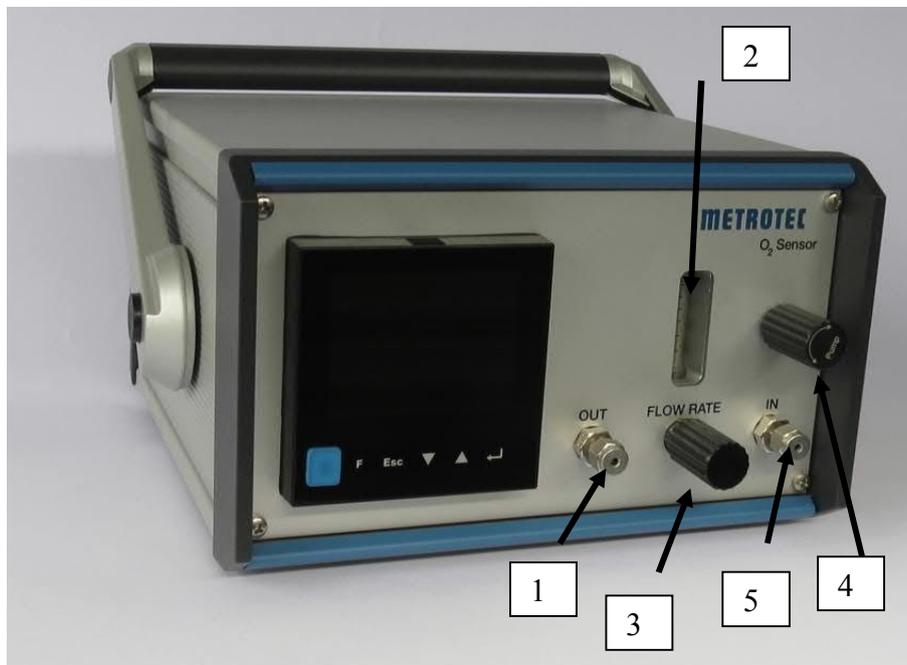

| | |
|---|--------------|
| 1 | Gas outlet |
| 2 | Flow meter |
| 3 | Bypass valve |
| 4 | Pump power |
| 5 | Gas inlet |

When the power supply to the measurement unit is switched on the sensor is heated for a period of 10 - 25 minutes to bring it up to the required minimum temperature.

NOTE: *During the heating-up period the unit does not indicate any useable values.*

When the gas inlet is opened and the gas pump is switched on, the unit should indicate 20.9 % O₂. If necessary, a correction can be made as detailed under "Correction" in the operating instructions.


The gas whose properties are to be measured is then fed to the sensor. The rate of flow should be within the green, background illuminated region of the flow meter and should never be allowed to exceed the range of the flow meter (this is a point of particular importance when the gas comes from a gas cylinder).

| |
|---|
| An excessive rate of flow could result in the destruction of the sensor |
|---|

The rate of flow can be set with the aid of the bypass valve and of the potentiometer that adjusts the delivery of the gas pump.

When the bypass valve is fully open the full flow of gas enters the measurement unit while a rate of flow some five times greater than occurs when the bypass valve is closed is constantly indicated.

4.3 Sketch of the ducting system

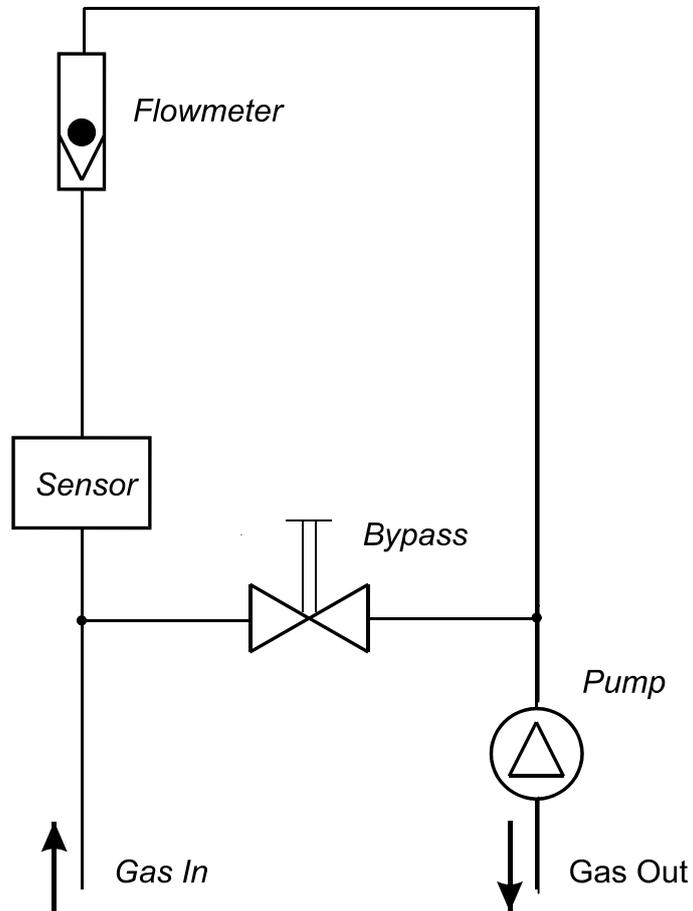

5 Putting the unit into operation

5.1 Switching the unit on

Once all electrical connections have been made and checked, the power plug is plugged in. After waiting for about 15 minutes for the sensor to be heated up, the unit indicates the oxygen content of the gas concerned. but stable values are only indicated about fifteen minutes after the heating-up period has expired.

5.2 Measurement

Once the switching-on operation is completed, the unit is ready for operation and the oxygen content of gases can be measured. As explained above, it is important to prevent the flow of gas exceeding the range covered by the flow meter.

5.3 Bottled gases

No special gas-treatment measures are called for when measuring the properties of such synthetic gases as nitrogen, argon, helium, etc. It is only necessary to provide for pressure reduction and precision dosing.

5.4 Process gases

5.4.1 General

It is not possible to give exact details of the measures needed for the avoidance of damage being done to the sensor and for correct pretreatment of all the many technical gases that may call for measurement but it is generally necessary for the gas to be free of dust and condensate and of any component that could suffer condensation. Such components could block the gas passages in the sensor result in it being damaged.

5.4.2 Hot process gases

If it is required to measure the properties of hot gases, the gas is withdrawn from the process and subjected to suitable treatment before being fed to the sensor. The withdrawal duct may be of metal or of ceramic material, depending on the temperature concerned. In most cases no special means of cooling is needed for the small amount of gas needed for measurement as it cools down on its own to around room temperature on its way to the measurement unit. It is important to avoid there being any leakage in the piping.

5.4.3 Special process gases

There are a great many processes in which the process gas contains components that generate liquid or solid condensate when beneath a certain temperature. Such condensates could be deposited in the gas passages in the sensor and affect the measurement results or cause the sensor to be damaged. Before starting to make measurements, it is recommended that the presence of such components be investigated and that steps be taken to filter out any that are found.

5.4.4 Location of condensate collectors

When fitting a condensate collection vessel, especially one for water, it should be ensured that it is located at the lowest point in the entire piping system..

It should be borne in mind that the filling of empty space in condensate collectors and filters will result in some delay in effecting measurements

5.4.5 Filter system arrangement:

The provisions made for the pretreatment of gases to be measured need to be adapted to the task concerned.

A standard system generally includes:

1. An initial water separator which may be equipped to empty itself of any condensate it may collect.
3. A coarse filter for the filtration of particles with a grain size exceeding 50 μ .
4. (Only necessary where a great deal of dust is involved)
5. A fine filter for the filtration of particles with a grain size exceeding 25 μ .
6. It is advantageous for this filter to be equipped to close off the gas flow immediately in the event of any liquid being applied to its filter element.

5.5 Switching off the measurement unit

It is preferable for the unit to be kept in continuous operation. As the sensor then remains heated there is less risk of it suffering the presence of condensation. that could lead to corrosion but if it is required to put the unit out of operation, the power plug should be withdrawn and attention be paid to the following points:

Heated sensors:

Inline sensors:

Remove carefully while still hot and allow to cool, taking care to avoid mechanical or thermal stress!

Compact sensors:

Flush with air before switching off

Unheated sensors:


These are generally left in place

Putting the measurement unit briefly out of operation:

When the unit is switched on again after being switched off for a short time, the instructions given above under "Switching the unit on" should be followed.


6 Operation

A few seconds after switching on, the first page is displayed as follows:

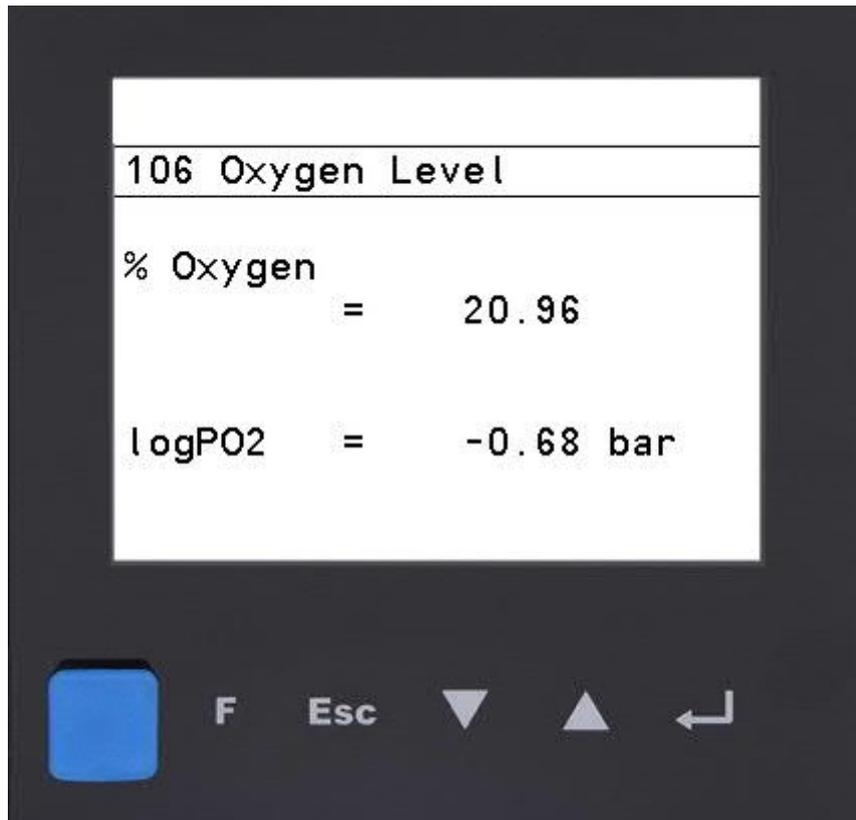

Each page has a headline that is separated by a line from the rest of the display. This headline indicates the page number and the title or an outstanding fault message. Beneath the line there is either a graph or a 6-line text.

The keypad has five components.

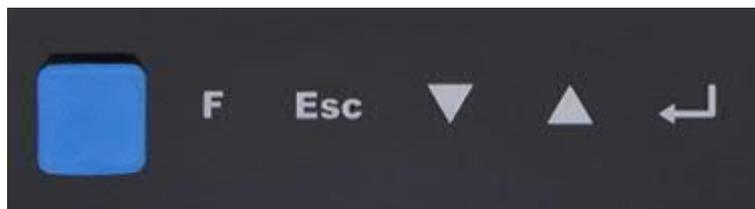

⇒ On the extreme left there is a rubber cap that is only removed to allow access to the socket beneath to which the communication cable is connected when it is required to install a new program.


⇒ The adjacent key provides for switching between manual and automatic operation.

- ⇒ The two arrow keys provide for moving the cursor line upwards or downwards or for increasing or decreasing values when alterations to entry fields are enabled.
- ⇒ The key on the right provides for
 - a) Opening a display page
 - b) Opening an entry field to enable an entry to be made
 - c) Closing an entry field and storing an entry.
- ⇒ The “Esc” key is for closing the display page or return to overview

Pressing the right-hand key causes the display to jump to the page selection list and then the cursor bar can be moved to the line bearing the required page title. When this no longer illuminated page title is confirmed by pressing the right-hand key, the page concerned is displayed.





An opened page can be closed again by pressing the right-hand key.



A window opens for any inputs. Like below example values can be stored by pressing the buttons. „Min“ and „max“ shows the limit values. „Cu“ shows the current value. Store by pressing „OK“.

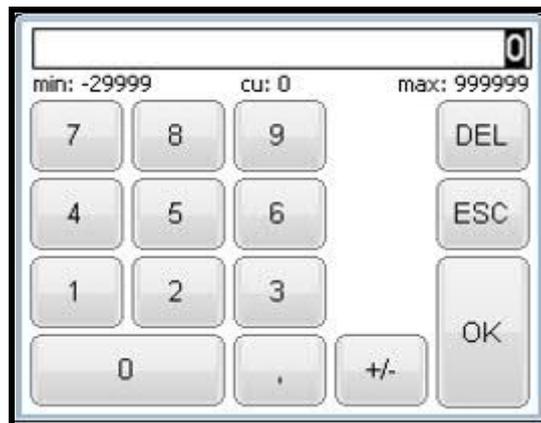

The various pages that can be selected in normal operation are detailed below.


| 107 P-Variables | | |
|-----------------|---|------------|
| EMF | = | 250 mV |
| Temp | = | 700 Grad C |
| logO2 | = | -5.47 bar |
| Dewp. | = | 100 Grad C |
| Lambda | = | 1.00 |
| O2 red | = | 9999 ppm |

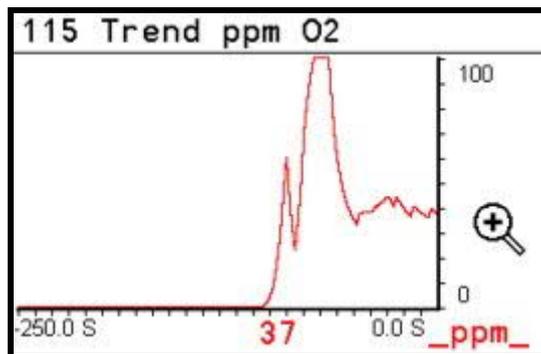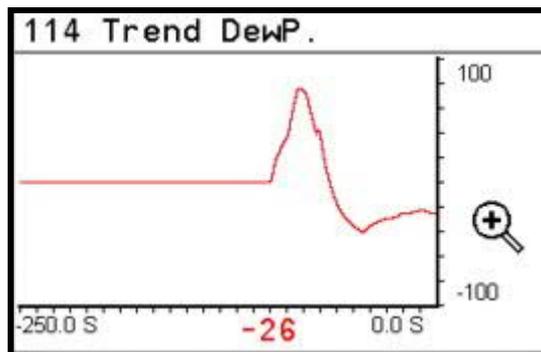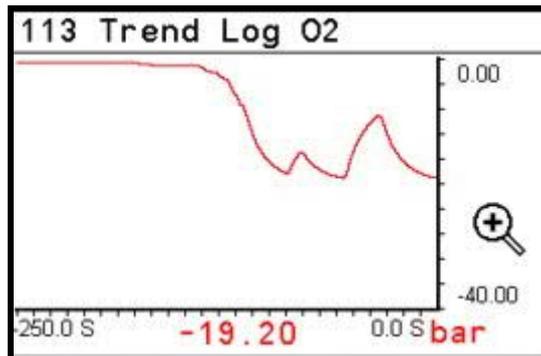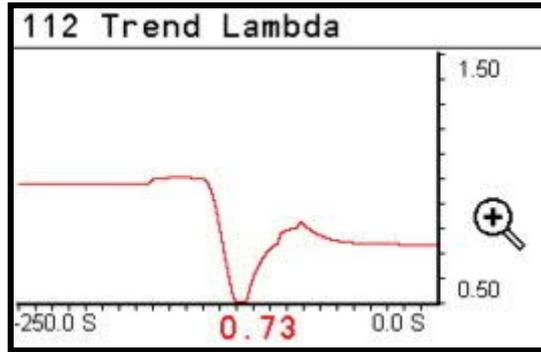

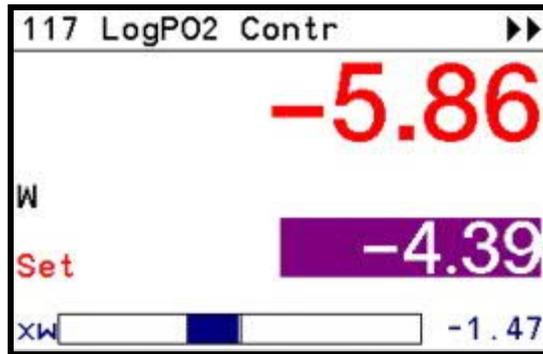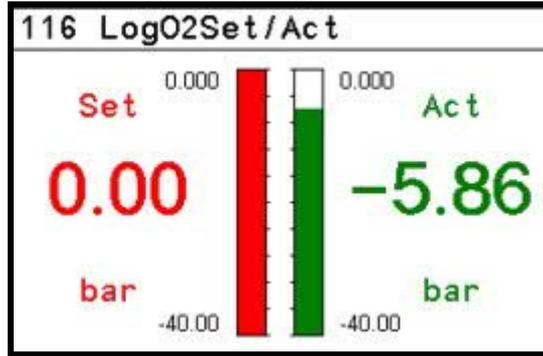


7 Configuration

7.1 Enablement of Configuration

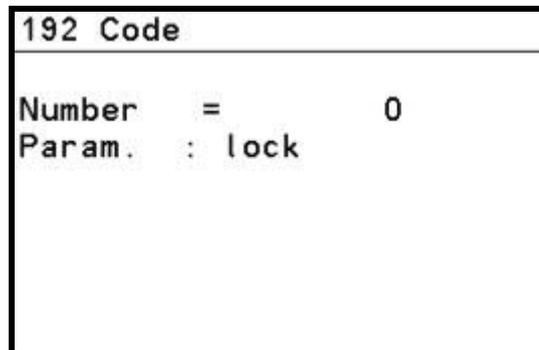

Before parameters can be altered it is first necessary to overcome the disablement code. Only then is access to additional pages possible. Enablement is effected as follows:

1. Select the page entitled CODE in the page selection table.
2. Press the key on the extreme right.
3. Keep pressing an arrow key until the NUMBER line is no longer backlighted.
4. Press the right-hand key. A input mask will open.

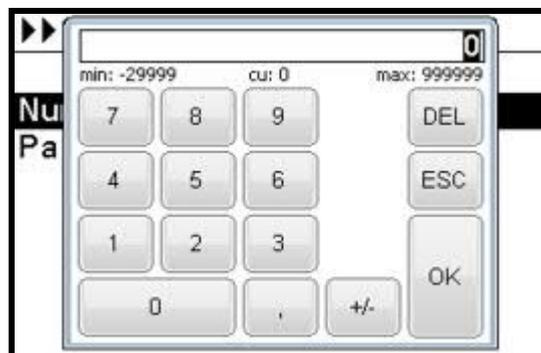

5. Press the right-hand key Press the right-hand key until your specific code (which was "1" on delivers) is displayed.
6. Once the required code is displayed, press the right-hand key once more to confirm the entry. The message "Parameters free" appears in the next line.

| | | |
|----------|---|------|
| 192 Code | | |
| Number | = | 0 |
| Param. | : | free |

You then have access to the page selection list once more.

| | | |
|-----------------|--------------|--|
| Operating pages | | |
| 106 | Oxygen Level | |
| 107 | P-Variables | |
| 112 | Trend Lambda | |
| 113 | Trend Log O2 | |
| 114 | Trend DewP. | |
| 115 | Trend ppm O2 | |
| 116 | LogO2Set/Act | |
| 117 | LogPO2 Contr | |

Note:

Access to parameters and configurations is enabled for only a limited period. (90 seconds) If more time is needed, then it will be necessary to repeat the steps needed to overcome the disablement code.

7.2 Displayed values


| | | |
|-----------------|---|------------|
| 119 Corrections | | |
| EMF + | = | 0.00 |
| EMF * | = | 1.00 |
| H2 Part. | = | 0.10 % |
| GasF. | = | 1.087 |
| LOG | = | -5.86 corr |
| O2 | = | 1.38 corr |

For the calculation of lambda and dew point it is necessary to enter characteristic values as also detailed under "Options".

Here you can adjust the measured value with an set point value of a test gas by varying “EMF+” or “EMF*”. The result is displayed under “LOG” and “O2”

The value 0.00 for the additive correction and of 1.0 for the multiplicative correction means that no correction is to be applied to the determined EMF value.

7.3 Process parameters

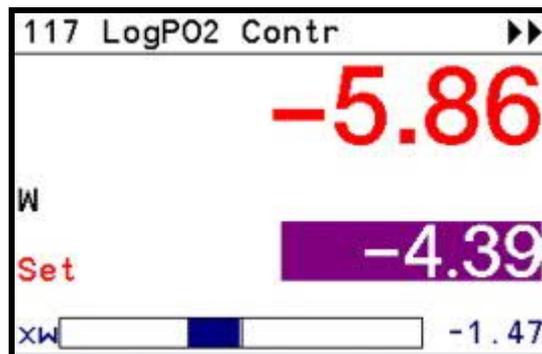

This page is selected from the page list as described above. The unlighted cursor beam can be positioned against the required value by means of the arrow keys. The cursor beam is then positioned against the value concerned and the entry is confirmed by pressing the right-hand key. The displayed value can be increased or decreased to cause the new required value to be displayed. Once this is achieved, it is confirmed by pressing the right-hand key and the new value is thus stored in the memory.

| 163 Contr.-Param | | |
|------------------|---|-------|
| Xp1 | = | 900.0 |
| Xp2 | = | 900.0 |
| Tn | = | 3.0 |
| Tv | = | 0.0 |
| Filter | = | 11.0 |

Filter = 0.0 means that no filter is active. Fluctuations in the sensor signal can be attenuated with the aid of a filter factor.

7.4 mA outputs

The device has three analogue outputs. Output 1 is for the logarithmic oxygen value, Output 2 for the linear oxygen value and Output 3 for various optional values such as dew point or

lambda: values for outputs 1 and 2 are thus displayed on one page and those for Output 3 on a separate page.

| 118 Out LIN/LOG | |
|------------------|---------|
| LINmax | = -3.00 |
| LOGmax | = 0.00 |
| LOGmin | = -6.00 |
|Output mA... | |
| = 4-20mA | |

The significance of LINmax values:

| | | | |
|-------|-----------|---------|-----------------|
| 0,00 | 10^0 | 1 | 100% |
| -1,00 | 10^{-1} | 0,1 | 10% |
| -2,00 | 10^{-2} | 0,01 | 1% |
| -3,00 | 10^{-3} | 0,001 | 0,1% = 1000 ppm |
| -4,00 | 10^{-4} | 0,0001 | 0,01% = 100 ppm |
| -5,00 | 10^{-5} | 0,00001 | 0,001% = 10 ppm |

It should be borne in mind that linear values always extend from 0 to LINmax and that with logarithmic values the LOGmax value must always be greater than LOGmin.

| 169 Scal. Out 3 | |
|--------------------|-------------|
| W: 0=L; 1=CO; 2=TP | |
| 3=O2B | |
| W: | = 2 Active |
| Part% of 0-100 | |
| up | = 100 20 mA |
| down | = 0 0/4 mA |

A choice has to be made between four possibilities. The figure "W" has to be set accordingly. End values have also to be set for 0 and for 20 mA. This is done by defining an end point within the total physical range for 0 – 100 parts indicated in the table below, within which a window for UPPER and LOWER limits can be established.

| | |
|-----------|---------------------|
| Lambda | 0 to 100 |
| CO | 0 to 10% |
| Dew point | -100 to 100 degrees |
| O2B | 0 to 1000 ppm |

7.5 Alarm output

| 128 Alarm Limits | | | |
|------------------|---|--------|--------|
| Limit Temp | | | |
| Max | = | 800 | Grad C |
| Min | = | 500 | Grad C |
| Limit logP02 | | | |
| Max | = | 0.00 | bar |
| Min | = | -30.00 | bar |

The definition of Alarm is self evident.

It has also to be defined whether the physical output is to be a relay or a semiconductor.

| 180 Lockout | | | |
|-------------|---|---|-------|
| Code | = | 1 | New |
| Code | = | 0 | I/O |
| Code | = | 0 | Konf. |
| Code | = | 0 | Comm. |
| Alarm is a | | | |
| Relay | | | |


7.6 Control output

It has also to be defined whether the physical control output is to be a relay or a semiconductor. If the alarm output is a relay then the control output is a semiconductor and if the alarm output is a semiconductor, then the control output is a relay.

| 180 Lockout | | | |
|-------------|---|---|-------|
| Code | = | 1 | New |
| Code | = | 0 | I/O |
| Code | = | 0 | Konf. |
| Code | = | 0 | Comm. |
| Alarm is a | | | |
| Relay | | | |

7.7 Scaling of the trend graphs

The scaling of the graphs cannot be altered. Alterations to the axes can only be effected by the supplier.

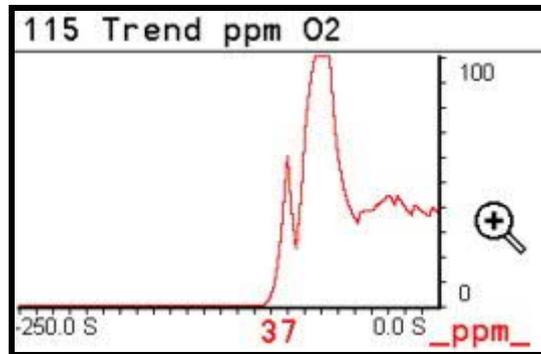

Exception: The Y-axis will be enlarged 4 times if „+“ will be pressed. Pressing „-“, the original scale is active again.

8 Options

8.1 Dew point

For some applications it is required that the dew point in degrees Celsius be calculated. This is frequently the case where nitrogen/hydrogen mixtures are concerned. The dew point is determined by comparing the measured O₂- value with that of a standard hydrogen percentage who's value has to be entered under "Parameters".

Note:

Calculation of dew point is a mathematical function. If there is a change in the hydrogen percentage or if no hydrogen is present, then the dew point cannot be calculated correctly

| 119 Corrections | | |
|-----------------|---|------------|
| EMF + | = | 0.00 |
| EMF * | = | 1.00 |
| H2 Part. | = | 0.10 % |
| GasF. | = | 1.087 |
| LOG | = | -5.86 corr |
| O2 | = | 1.38 corr |

8.2 Lambda


For some applications it is of importance to know the lambda value of a combustion gas or of a gas/air mixture. In this case, lambda is defined as follows:

$$\text{Lambda} = (\text{combustion air supplied}) / (\text{combustion air theoretically required})$$

If this feature is required, it is necessary for a characteristic value to be entered in the "Parameter" menu.

Note:

Calculation of dew point is a mathematical function. If the C/H value changes or is not present, then the lambda value can no longer be calculated correctly

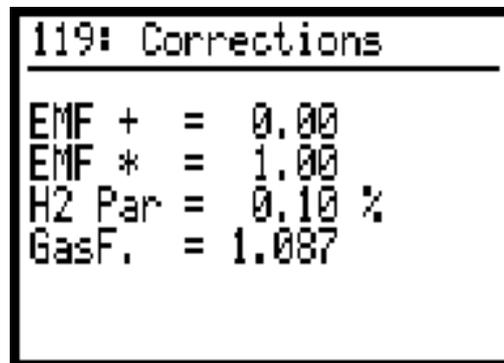

| 119: Corrections | |
|------------------|----------|
| EMF + | = 0.00 |
| EMF * | = 1.00 |
| H2 Par | = 0.10 % |
| GasF. | = 1.087 |

8.3 CO

The CO value is derived from the lambda function. (see note under lambda)

8.4 Calculated oxygen value

The calculated oxygen value "O2B" of a nitrogen/hydrogen mixture is determined from the hydrogen percentage (see under "Dew point" option)

9 Interfaces

9.1 Analog interfaces

The device has three 0 – 20 mA analogue interfaces all of which can be active at the same time. A change to 4 – 20 mA can be effected by the user.

| 118 Out LIN/LOG | |
|------------------|---------|
| LINmax | = -3.00 |
| LOGmax | = 0.00 |
| LOGmin | = -6.00 |
|Output mA... | |
| = 4-20mA | |

9.2 Digital interfaces


9.2.1 Standard interfaces

There are two relays, either of which can be defined as either a control output or as an alarm output. There are also two semiconductor outputs which can be defined as an alarm or as a control output.

| 180 Lockout | |
|-------------|-----------|
| Code | = 1 New |
| Code | = 0 I/O |
| Code | = 0 Konf. |
| Code | = 0 Comm. |
| Alarm is a | |
| Relay | |

9.2.2 Optional interface: RS 485

The interface plug is at rear site between the connector block

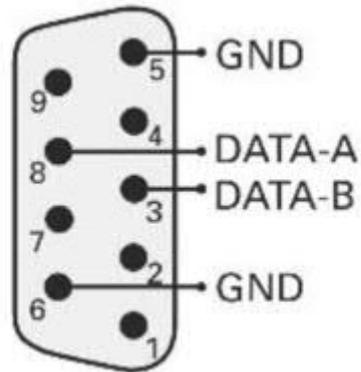

| 180 Lockout | |
|-------------|-----------|
| Code | = 1 New |
| Code | = 0 I/O |
| Code | = 0 Konf. |
| Code | = 0 Comm. |
| Alarm is a | |
| Relay | |

To define the interface it first must be entered at "Lockout" the code 5 in line "Comm". Then skip to the definition-page with 2 times pressing the "Esc" button. Following the interface-parameters like type, address and baurate can be defined.

| |
|------------------------|
| Main menu |
| Operating pages |
| Parameter |
| Signals |
| Configuration |
| Device settings |
| |

| |
|-----------------|
| Device settings |
| Date, time |
| Device data |
| Online/Offline |
| Calibration |
| Info |
| Status I/O |
| Status CAN-Bus |

| |
|-------------------|
| Device data |
| Protoc = ISO 1745 |
| Baud = 4800 |
| Addr. = 1 |
| Frequ. = 50 Hz |
| Langu. = english |
| CAN-Id = (NMT) 1 |
| CAN-Bd = 20kBit |
| Freeze = off |

Data request at protocol ISO 1745, 7bit, 1 Stopbit, Even, for the example address 1 is:
Whereat: Addr = address, C3 ...C6 und C1 are invariable,

| Value for C2 | |
|--------------|----------------------|
| 3 | = % O ₂ |
| 4 | = Log O ₂ |
| 5 | = ppm O ₂ |
| 6 | = Tp |
| 7 | = O ₂ red |
| 8 | = Temperature |
| 9 | = Alarm |

Whereat alert 1 = faultless, 2 = collective message, 3 = range overstepping 4 = collective message and range overstepping

| | | | | | | | | | | | | |
|-----|-----|-----|----|----|----|----|----|----|----|----|-----|--|
| EOT | Adr | Adr | C1 | C2 | , | C3 | C4 | C5 | , | C6 | ENQ | |
| EOT | 0 | 1 | 0 | 0 | , | 0 | 0 | 1 | , | 0 | ENQ | |
| 04 | 30 | 31 | 30 | 33 | 2C | 30 | 30 | 31 | 2C | 30 | 05 | |

Response

| | | | | | |
|-----|----|------|----|----------|-----|
| STX | C1 | C2+1 | = | Wert | EOT |
| STX | 0 | 1 | = | Wert | EOT |
| 04 | 30 | 34 | 3D | HEX-Wert | 05 |

Data request at protocol Modbus RTU, 8bit, 1 Stopbit, Even

| Device data | |
|-------------|---------|
| Protoc = | Modbus |
| Baud = | 19200 |
| Addr. = | 1 |
| Frequ. = | 50 Hz |
| Langu. = | english |
| CAN-Id = | (NMT) 1 |
| CAN-Bd = | 20kBit |
| Freeze = | off |

| Adress | Function | Storage adress | | Registers | | CRC 1 | CRC 2 |
|--------|----------|----------------|-------|-----------|-------|-------|-------|
| | | Byte1 | Byte2 | Byte1 | Byte2 | Byte | Byte |
| | 03 | | | | | | |

Excample for a request at address 1 in HEX-display

| Measurement value | | | | | | | | |
|--------------------|----|----|----|----|----|----|----|----|
| % O ₂ | 01 | 03 | 80 | A4 | 00 | 02 | AC | 2B |
| log O ₂ | 01 | 03 | 80 | A6 | 00 | 02 | 0D | E8 |
| ppm O ₂ | 01 | 03 | 80 | A8 | 00 | 02 | 6C | 2B |
| TP | 01 | 03 | 80 | AA | 00 | 02 | CD | EB |
| O ₂ red | 01 | 03 | 80 | AC | 00 | 02 | 2D | EA |
| Temperature | 01 | 03 | 80 | AE | 00 | 02 | 8C | 2A |
| Alarm | 01 | 03 | 80 | B0 | 00 | 02 | EC | 2C |

| | | | | | | | | |
|------------|----|----|----|----|----|----|----|----|
| All values | 01 | 03 | 80 | A4 | 00 | 0E | AC | 2D |
|------------|----|----|----|----|----|----|----|----|

Excample for the request:

| | | | | | | | | |
|-------------|----|----|----|----|----|----|----|----|
| Temperature | 01 | 03 | 80 | AE | 00 | 02 | 8C | 2A |
|-------------|----|----|----|----|----|----|----|----|

Excample-answer = 1760,00

| | | | | | | | | | |
|-------------|----|----|-------|-------|-------|-------|-------|----|----|
| Temperature | 01 | 03 | 04 | 44 | DC | 00 | 00 | 2F | 39 |
| | | | 4Byte | Byte1 | Byte2 | Byte3 | Byte4 | | |

9.2.3 Optionale interface: Ethernet

The interface plug is at rear site between the connector block.
Connection to network is done by standard cables.

| 180 Lockout | | |
|---------------------|---|---------|
| Code | = | 1 New |
| Code | = | 0 I/O |
| Code | = | 0 Konf. |
| Code | = | 0 Comm. |
| Alarm is a Relay | | |

To define the interface it first must be entered at "Lockout" the code 5 in line "Comm". Then skip to the definition-page with 2 times pressing the "Esc" button. Following the interface-parameters like type, address can be defined.

| |
|------------------------|
| Main menu |
| Operating pages |
| Parameter |
| Signals |
| Configuration |
| Device settings |
| |

| |
|--------------------|
| Device settings |
| Date, time |
| Device data |
| Online/Offline |
| Calibration |
| Info |
| Status I/O |
| Status CAN-Bus |

```

Device data
Frequ. =          50 Hz
Langu. =          english
CAN-Id =          (NMT) 1
CAN-Bd =          20kBit
Freeze =          off
Delay =           0
Ethernet
    
```

```

IP-Addr = 192.168.000.051
Subnet  = 255.255.255.000
Gateway = 192.168.000.001
DHCP    = off
MAC-Adr = 00-0F-67-0F-4C-8C
Loc host= KS98-2_0F-4C-8C
    
```

Input for IP-address und Subnet.

The data protocol is similar Modbus protocol which is explained above

| Modbus RTU Message | | | | | | |
|--------------------|-------------|--------|----------|-----------------------|------|-------|
| | | | Slave ID | FCode | Data | CRC |
| Modbus TCP/IP | | | | | | |
| Header | | | | Modbus TCP/IP Message | | |
| Transaction ID | Protocol ID | Length | Unit ID | FCode | Data | |
| Example | | | | | | |
| 0005 | 0000 | 0006 | 01 | 010380A4 | 000E | ----- |

10 Special features

10.1 Correction factors

There is one additive and one multiplicative correction factor. These can be applied as a correction to the EMF value determined by the sensor and thus to the measured value that is displayed. It may be necessary to amend these factors in the course of calibration. The necessary entry is detailed under "Configuration".

| 119 Corrections | | |
|-----------------|---|------------|
| EMF + | = | 0.00 |
| EMF * | = | 1.00 |
| H2 Part. | = | 0.10 % |
| GasF. | = | 1.087 |
| LOG | = | -5.86 corr |
| O2 | = | 1.38 corr |


10.2 Filter factor

If there is excessive fluctuation in the measured values, it is possible to apply an attenuation factor of between 0 and 200. This attenuation factor has an integration effect on the oxygen value. The necessary entry is detailed under "Configuration Process parameters".

| 163 Contr. -Param | | |
|-------------------|---|-------|
| Xp1 | = | 900.0 |
| Xp2 | = | 900.0 |
| Tn | = | 3.0 |
| Tv | = | 0.0 |
| Filter | = | 11.0 |

10.3 Oxygen controller

The required value is entered as the logarithmic oxygen partial pressure
The necessary entry is detailed under "Configuration Process parameters".

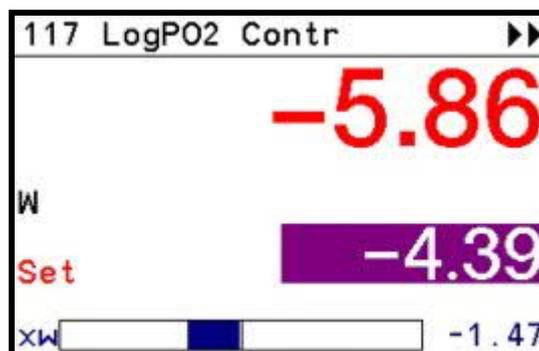

10.4 Coding

To prevent unauthorised amendment of important entries, the pages concerned are only displayed once an access code has been entered (see under "Enablement of configuration")
On this page there is provision for programming a new access code.

Caution:

Not even the supplier can decipher an access code that has been forgotten.

THE PROBLEM CAN ONLY BE SOLVED BY ENTERING COMPLETELY NEW SOFTWARE:

```
180 Lockout
Code      =      1 New
Code      =      0 I/O
Code      =      0 Konf.
Code      =      0 Comm.
Alarm is a
Relay
```

10.5 Function of the clock


First line displays the time. The time hasn't any function inside of the program. If the time should be adjusted it should be done like described for the interface

```
Device settings
Date, time
Device data
Online/Offline
Calibration
Info
Status I/O
Status CAN-Bus
```

11 Technical data

| | |
|-------------------------------------|--|
| Measurement range | 100 % to 10 ⁻³¹ bar O ₂ |
| Ambient temperature | 0 to 45 degrees Celsius |
| Measurement accuracy | +/- 0.3 mV of the sensor EMF +/- 2 degrees Celsius +/- 2% of the mA output +/- 2% of the log oxygen partial pressure |
| Temperature input | Thermocouple Type S |
| Heating-up time for sensors | 10 to 15 minutes |
| Response time | approx 2 seconds |
| Contact load capacity | 2A, 24 V (ohmic) |
| Dimensions | 160 x 260 x 260 mm (HxWxD) |
| Electromagnetic compatibility | The equipment meets the requirements of European directive 89/336EWG and complies with the following standards: Interference transmission EN 61000-6-2 Immunity from interference EN 61000-6-4 The device can be used without restriction in residential and industrial surroundings. |
| Power supply | 230 Volt AC |
| Heating power | approx.. 200 VA |
| Control power | approx. 40 VA |
| Temperature of the measurement cell | 700 °C |
| Temperature detection element | Thermocouple Pt 10Rh-Pt |
| Temperature of measurement gas | max. 50 °C |
| Flow of measurement gas required | At least 8 litre per hour with bypass closed |
| Moisture | Dew point must be filtered out. It is important to avoid presence of condensate |
| Dust | Dust must be filtered out Solid particles exceeding 25 µ must be filtered out |
| | |

12 Connection plan

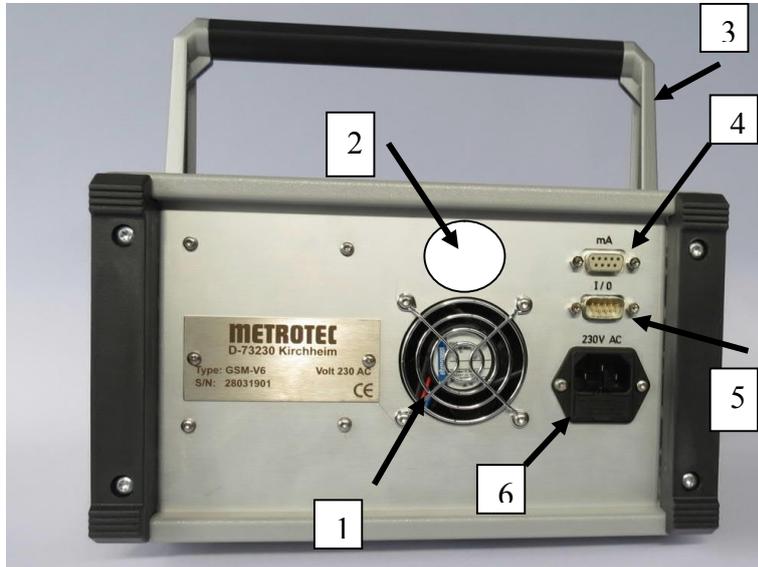

| | |
|---|-------------------------------------|
| 1 | Fan |
| 2 | Optional plug for Ethernet or RS485 |
| 3 | Handle |
| 4 | mA- outputs |
| 5 | Conductor outputs |

| | Standard | Standard | Option | Option |
|-----------------|---------------------|----------------------|---------------------|-------------|
| PIN | 9-pin. DSUB „mA“ | 9-pin DSUB „I/O“ | 9-pin DSUB „RS 485“ | Ethernet |
| Plug “unit” | female | male | female | RJ45 female |
| 1 | Output 3 - | Alarm „c“ | | |
| 2 | Oxygen linear - | „nc“ | | |
| 3 | Oxygen logarithm. - | „no“ | Data B | |
| 4 | | | | |
| 5 | | | GND | |
| 6 | Output 3 + | Controller/Alarm „c“ | GND | |
| 7 | Oxygen linear + | „nc“ | | |
| 8 | | „no“ | Data A | |
| 9 | Oxygen logarithm. + | | | |
| Plug unit“ „for | male | female | male | RJ45 male |